


PCTWORLD INTELLECTUAL PROPERTY ORGANIZATION
International Bureau

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶: H04R 25/00	A1	(11) International Publication Number: WO 96/21334 (43) International Publication Date: 11 July 1996 (11.07.96)
(21) International Application Number: PCT/US95/17113 (22) International Filing Date: 27 December 1995 (27.12.95) (30) Priority Data: 08/365,913 29 December 1994 (29.12.94) US (71) Applicant: DECIBEL INSTRUMENTS, INC. [US/US]; 3857 Breakwater Avenue, Hayward, CA 94545 (US). (72) Inventors: SHENNIB, Adnan; 34337 Xanadu Terrace, Fremont, CA 94555 (US). URSO, Richard; 15 Bennet Road, Redwood City, CA 94063 (US). (74) Agent: GLENN, Michael, A.; P.O. Box 7831, Menlo Park, CA 94026 (US).		(81) Designated States: AM, AU, BB, BG, BR, BY, CA, CN, CZ, DK, ES, FI, GE, HU, JP, KG, KP, KR, KZ, LK, LT, LV, MD, MG, MN, NO, NZ, PL, RO, RU, SI, SK, TJ, TT, UA, UZ, VN, ARIPO patent (KE, LS, MW, SD, SZ, UG), European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i>

(54) Title: ARTICULATED HEARING DEVICE**(57) Abstract**

A hearing device (10) having highly articulated, non-contiguous parts and adapted for placement within the ear canal (20) includes a receiver module (40) for delivering acoustic signals within close proximity to the tympanic membrane (26), a main module (12) containing all hearing aid components except the receiver, and a connector (50) that routes amplified electrical signals from the main module (12) to the receiver module (40). The connector (50) fits in the cartilaginous area (28) of the ear canal (20) and is articulated with both the receiver module (40) and main module (12) to permit independent movement of the receiver module (40) while the hearing device (10) is inserted or removed and during various jaw movements, such as chewing, yawning and talking.

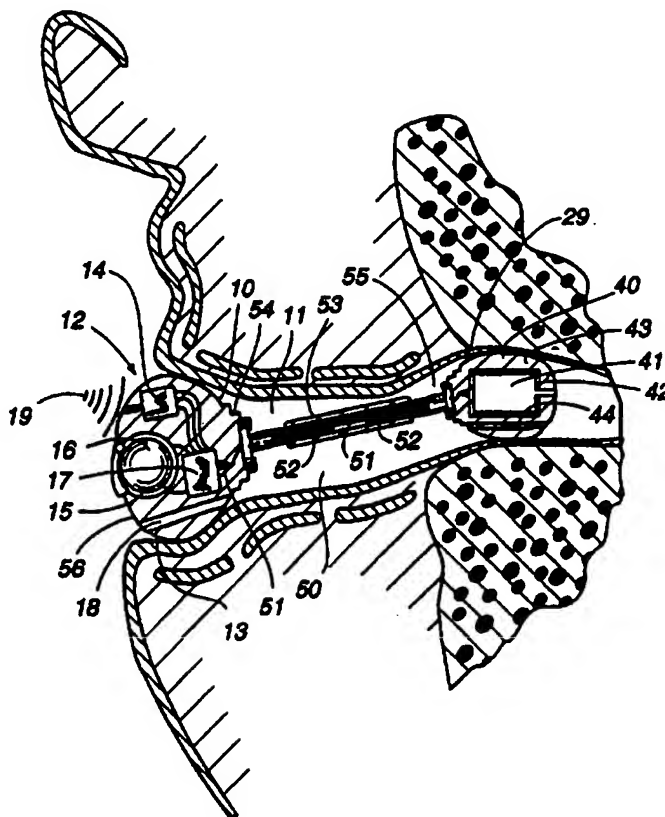

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AM	Armenia	GB	United Kingdom	MW	Malawi
AT	Austria	GE	Georgia	MX	Mexico
AU	Australia	GN	Guinea	NE	Niger
BB	Barbados	GR	Greece	NL	Netherlands
BE	Belgium	HU	Hungary	NO	Norway
BF	Burkina Faso	IE	Ireland	NZ	New Zealand
BG	Bulgaria	IT	Italy	PL	Poland
BJ	Benin	JP	Japan	PT	Portugal
BR	Brazil	KE	Kenya	RO	Romania
BY	Belarus	KG	Kyrgyzstan	RU	Russian Federation
CA	Canada	KP	Democratic People's Republic of Korea	SD	Sudan
CF	Central African Republic	KR	Republic of Korea	SE	Sweden
CG	Congo	KZ	Kazakhstan	SG	Singapore
CH	Switzerland	LI	Liechtenstein	SI	Slovenia
CI	Côte d'Ivoire	LK	Sri Lanka	SK	Slovakia
CM	Cameroon	LR	Liberia	SN	Senegal
CN	China	LT	Lithuania	SZ	Swaziland
CS	Czechoslovakia	LU	Luxembourg	TD	Chad
CZ	Czech Republic	LV	Latvia	TG	Togo
DE	Germany	MC	Monaco	TJ	Tajikistan
DK	Denmark	MD	Republic of Moldova	TT	Trinidad and Tobago
EE	Estonia	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	UG	Uganda
FI	Finland	MN	Mongolia	US	United States of America
FR	France	MR	Mauritania	UZ	Uzbekistan
GA	Gabon			VN	Viet Nam

Articulated Hearing Device

BACKGROUND OF THE INVENTION

5

TECHNICAL FIELD

10 The invention relates to hearing aids. More particularly, the invention relates to hearing devices that can be easily and deeply inserted in the ear canal, while accommodating deformations of the ear canal to provide a comfortable fit.

DESCRIPTION OF THE PRIOR ART

15

The trend in the design and manufacture of hearing devices has generally been towards miniaturization as device components and energy sources continue to decrease in size and improve in efficiency. This trend is largely fueled by the demand for a more inconspicuous and cosmetically appealing devices to avoid the stigma of aging and disability associated with hearing impairment.

20 Two decades ago, hearing devices were predominately of the Behind-The-Ear (BTE) type. These devices are placed behind the ear with an acoustic tube connecting the device to an ear mold placed within the ear. Today, smaller In-The-Ear (ITE) type devices which essentially fit within the concha of the ear, represent the largest segment of hearing aid types used. Smaller In-The-Canal (ITC) types, which fit partially in the concha and partially within the ear canal, have also become increasingly popular in recent years. In concert with this miniaturization trend, smaller hearing aid devices that fit completely within the ear canal, known as Completely-In-the-Canal (CIC), are now offered on the market.

30 In addition to the obvious cosmetic advantages of miniature hearing devices, *e.g.* ITC and CIC types, there are several other advantages that result from device placement within the ear canal. These advantages include improved high frequency response, reduced distortion, reduced occlusion effect, improved sound localization, reduced wind noise, fewer wax problems that

typically plug the device receiver, improved use with telephones, and improved overall sound fidelity due to reduced residual volume in the ear canal and proximity of the hearing device receiver to the tympanic membrane (for example, see Gudmundsen, G.I., *Fitting "CIC" Hearing Aids-Some Practical Pointers*, The Hearing Journal, vol. 47, No. 7, 1994, pp. 10, 45-48; and Agnew, J., *Acoustic Advantages of Deep Canal Hearing Aid Fittings*, Hearing Instruments. Vol. 45, No. 8, 1994, pp. 22-25).

Anatomy and Morphology of the Ear Canal

10

Figs. 1 and 2 show a cross-sectional anatomical view of the ear in the coronal and transverse planes of the head, respectively. The ear, for the purpose of this invention, can be described as having three segments. The first segment represent the medial concha cavity 20 just behind the tragus 21 which is relatively large and is surrounded by cartilaginous tissue 22. The second cavity 23, medial to the aperture 24 of the external acoustic meatus 11, is generally smaller and is also surrounded by cartilaginous tissue 22. The third cavity 25 defines the final canal segment near the tympanic membrane 26 and is surrounded by dense bony tissue 27. The tissue covering the cartilaginous regions 28 is relatively thick and has a well developed subcutaneous layer thus allowing some expansion to occur. In contrast, the tissue covering the bony region 29 is relatively thin and therefore, little or no tolerance for expansion exists in this region. The cartilaginous region 23 is the major area of cerumen production and accumulation in the ear canal.

The shape of a typical external ear canal, unlike that shown in most artistic renderings, is rarely cylindrical or conical with a gradual narrowing towards the tympanic membrane. Instead, most ear canals are non-uniform and have various levels of tortuous contours. Some canals have severe restrictions in the cartilaginous area.

The ear canal is generally S-shaped, with a first bend 30 occurring approximately at the aperture of the ear canal and a second bend 31 occurring at the cartilaginous-bony junction. The cross sectional diameter of the ear canal and the orientation of various regions within the canal are known to vary considerably from one individual to another. For example, the length from the aperture 24 to the lateral edge 32 of tympanic membrane 26 ranges from about 20 mm to about 25 mm. The cross sectional shape is

generally oval. The smallest diameter is generally in the bony region 29 in the transverse plane and ranges from about 4 mm to about 7 mm. The largest diameter is in the medial concha region 20 in the coronal plane and ranges from about 10 mm to about 18 mm.

5

The morphology of the ear canal reveals substantial deformation within the cartilaginous area 23 of the ear canal as a result of mandibular motion associated with talking, chewing, yawning, and biting. This deformation is generally caused by the asymmetric stresses from the actions of the mandibular condyle 33 (see Fig. 2) on neighboring cartilaginous tissue. These deformations have radial components, *e.g.* constrictions, and axial components, *i.e.* inward and outward motion. These radial and axial deformations can generally be felt when one inserts a finger in the ear canal and moves the jaw. In one study, using magnetic resonance imaging (MRI), the deformation was shown to be as much as 25% in the anterior-posterior direction of the cartilaginous region of the canal (see, for example Oliveira, R.J., Hammer, B., Stillman, A., Holm, J., Jons, C., Margolis, R.H., *A Look at Ear Canal Changes with Jaw Motion*, Ear and Hearing, Vol. 13, No. 6, 1992, pp. 464-466).

20

The unique and tortuous nature of individual ear canals, in combination with the dynamic canal deformations due to mandibular motion, present unsolved challenges to users of current hearing aid designs, particularly for deep canal devices. These problems include difficulty in device insertion and removal, discomfort, device retention, and oscillatory feedback. These problems are further aggravated for persons who suffer abnormal mandibular function leading to severe ear canal deformations, as in the case of temporal mandibular joint (TMJ) syndrome.

30 The State of the Art

The substantial inter-subject variability of ear canal shapes has lead the hearing aid industry to develop hearing devices that are custom manufactured, based on individual ear canal impressions sent to the manufacturer by the dispensing professional. These custom devices require an accurate impression to fabricate hearing devices that precisely conform to the shape of the ear canal. This custom fit attempts to minimize discomfort to the patient and possible damage to the patient's ear tissue and to prevent feedback-causing acoustic leakage (see, for example Staab, W.J., Martin,

35

L.R., *Taking Ear Impressions for Deep Canal Hearing Aid Fittings*, The Hearing Journal, Vol. 47, No. 11, 1994, pp. 19-28).

- Previews of available miniature devices (see, for example *Special Report: Completely-In-The-Canal Hearing Instruments*, The Hearing Journal, Vol. 47, No. 11, 1994, pp. 56-57; and *Mini-Canal Hearing Instruments In Review*, Hearing Instruments, Vol. 40, No. 1, 1989, pp. 30-36, 52) reveal an assortment of hearing devices that require individualized ear impressions and custom manufacturing. These custom hearing devices are generally made of rigid or semi-rigid acrylic material. Although they may conform to the shape of the ear canal when they are fully inserted, they present insertion and removal difficulties, particularly for individuals having tortuous canals and canals that have non-gradual narrowing.
- Non-custom hearing devices, e.g. stock hearing aids that do not require individual ear canal impressions or custom manufacturing, have been also available on the market. For example, the E-Z EAR hearing device manufactured by General Instruments, Inc., New Orleans, LA is a stock hearing device that is marketed as a loaner or a back-up device, because a precise fit of a custom device is considered important for patient comfort and feedback considerations with current hearing aid designs.

- Another stock hearing device is described by Veroba *et al* (see U.S. patent No. 4,870,688), in which a rigid core module containing electronic components is combined with a malleable covering module. The modules are selected from an off-the-shelf assortment to personalize the device fit. Even though the covering is malleable, the core module is rigid and the combined structure has a contiguous housing that has only limited ability to conform to various non-uniform ear canal shapes of a broad population. This is especially true for hearing devices that are deeply inserted in ear canals that are typically S-shaped.

- Another attempt to resolve the problem of conforming a hearing device to the unique shapes of individual ear canals is disclosed in Oliveira, R.J., *Better Hearing Instruments Through Chemistry*, Hearing Instruments, Vol. 39, No. 10, 1988. Oliveira proposed attaching a compressible foam ear mold to the acoustic output of ITE and ITC hearing aids containing a receiver via a threaded coupler. The foam ear mold contains a semi-rigid tubing that prevents the foam from fully collapsing and occluding the sound intended for

delivery to the tympanic membrane. The overall length of the device and the fixed relationship between the foam ear mold and the hearing device renders this solution impractical for dealing with various ear canal shapes and sizes, particularly for deep ear canal device insertion.

5

Sciarra, M. (see U.S. patent No. 4,539,440) describes an ITC hearing device having a generally cylindrical body with a resilient stretchable outer layer that is adjustable to expand and change the diameter of the device. The device is adjustably expandable such that it fits snugly within the ear canal and is flexibly hinged to permit axial flexibility to accommodate the curvature of the ear canal. However, Sciarra fails to teach how an essentially cylindrical shaped device conforms to ear canals that are generally non-uniform or that are S-shaped.

15 Biermans, J. (see U.S. patent No. 4,937,876) describes a hearing device that consists of two units. The first unit has a larger cross section and contains typical hearing aid components, except for the receiver. The second unit has a smaller diameter and contains the receiver. The two units, which may either be contiguous or separated, are encapsulated by a
20 contiguous housing, presumably of standard rigid or semi-rigid acrylic material.

Painter, D.S. *et al* (see UK patent No. GB 2 203 379 A) describes a non-custom hearing device that initially contains a flexible membrane housing.
25 The device is inserted into the ear canal and a curable material is injected into the flexible housing, causing the device to harden while conforming to the shape of the ear canal. Arndt, H. (see U.S. patent No. 5,201,008) describes a modular hearing device having a housing that includes a hinged face-plate. The housing contains modular electronic and receiver
30 components. The housing, *e.g.* hearing aid shell, may be custom or stock. Stanton, M. (see U.S. patent No. 5,185,802) describes a modular hearing device having a removable universal interior module that fits within an exterior shell which is customized for right or left ear canals.

35 The above mentioned designs of miniature hearing devices, *e.g.* ITC and CIC, whether fully custom manufactured or stock manufactured for off-the-shelf dispensing, modular or non-modular, having rigid, semi-rigid, or malleable housing, do not deal effectively with typical ear canal deformations that are due to various jaw movements. These dynamic

deformations in the cartilaginous area lead to many undesirable effects that are known in the hearing aid industry, including poor device retention due to axial pressures on the device, discomfort, pain, and acoustic oscillatory feedback.

- 5
- Ward, L.W. *et al* (see U.S. patent nos. 5,201,007 and 5,031,219) describes a hearing aid having a rigid acoustic conduction tube that conducts sounds to the tympanic membrane. The acoustic conduction tube has an external diameter that is smaller than the ear canal and a flexible flanged tip that
- 10 seals near the tympanic membrane. This concept, which is known as minimal contact technology (MCT), alleviates some of the stresses caused by ear canal deformation via the narrow sound conduction tubing which is in minimal contact with the tissue that is subject to deformation. The practical implementation of this concept is described for BTE and ITE types, for
- 15 example, by Bryant, M. Mueller, H.G., Northern, J.L., *Minimal Contact Long Canal "ITE" Hearing Instruments*, Hearing Instruments, Vol. 42, No. 1, 1991, pp. 12-15, 48. However, the applicability of the MCT concept is questionable for conventional miniature hearing device designs, *e.g.* ITC or CIC. Such hearing devices have a contiguous rigid or semi-rigid housing,
- 20 and may not be comfortably and deeply inserted into a narrow and tortuous ear canal.

SUMMARY OF THE INVENTION

- 25 The invention provides a hearing device that incorporates all of the known advantages of miniature hearing aids that are deeply inserted in the ear canal with new designs that greatly facilitate device insertion and removal, while also providing a hearing device having comfortable fit, and reduced oscillatory feedback during normal and abnormal ear canal deformation.

30 The invention provides a hearing device having non-contiguous parts that are highly articulated within the ear canal. The device primarily consists of three main modules:

- 35 (1) A receiver module that delivers acoustic signals within close proximity of the tympanic membrane;
- (2) A main module essentially containing typical hearing aid components, except the receiver; and

(3) A connector that routes the amplified electrical signals from the main module to the receiver module.

- 5 The connector fits in the cartilaginous area of the ear canal and is articulated with both the receiver and main modules to accommodate essentially independent movement of the receiver and main modules when the hearing device is inserted or removed, and during various jaw movements such as chewing, yawning, and talking. The connector may be an adjustable shaft to
10 accommodate various ear canal lengths and to allow for incremental receiver depths within the ear canal.

The receiver module is inserted deeply into the ear canal, preferably in the bony portion of the ear canal, to provide all of the advantages associated
15 with deep receiver placement. These advantages include improved energy efficiency and high frequency response, reduced oscillatory feedback, reduced occlusion effect, reduced distortion, and reduced perceived noise. The receiver module includes various seals that substantially reduce acoustic leakage that can cause oscillatory feedback. Furthermore, because
20 the receiver module is completely encapsulated and essentially isolated from the microphone in the main module, internal acoustic leakage that can cause oscillatory feedback is also reduced.

In the preferred embodiment of the invention, the main module is loosely
25 fitted in the medial concha area just behind the tragus. The hearing device is generally invisible unless viewed directly from the side of the ear. The main module can be highly vented with minimal concerns for oscillatory feedback. This venting allows occluded own-sounds, *i.e.* sounds that originate with the individual wearing the device, resonating in the
30 cartilaginous cavity to leak out of the hearing aid, instead of propagating to the tympanic membrane, as is the case in conventional hearing aids which have a single contiguous enclosure.

In the preferred embodiment of the invention, the receiver module may
35 connect to any of an assortment of acoustic seal tips to accommodate variability in ear canal diameters and shapes. The unique features of the invention, for example articulated parts, adjustable connector length, and assorted acoustic seal tips, provide a universal hearing device that can be

dispensed at the point of sale without the need for ear canal impressions or custom manufacturing.

BRIEF DESCRIPTION OF THE DRAWINGS

5

Figure 1 is an anatomical view of a right ear in the coronal plane;

Figure 2 is an anatomical view of a right ear in the transverse plane;

- 10 Figure 3 is a coronal plane view of a right ear showing an articulated hearing device in accordance with the invention;

Figure 4 is a transverse plane view of a right ear showing an articulated hearing device in accordance with the invention;

15

Figure 5 is a view of an articulated hearing device showing response to radial and axial deformations in the transverse plane in accordance with the invention;

- 20 Figures 6a and 6b show a pediatric size main module housing in accordance with the invention;

Figures 7a and 7b show an adult size main module housing in accordance with the invention;

25

Figures 8a and 8b show a large size main module housing in accordance with the invention;

- 30 Figures 9a and 9b provide coronal and transverse views, respectively, of articulated device modules showing module articulation and general dimensions in accordance with the invention;

Figure 10 is a sectioned view of a receiver module having a built-in soft and compliant housing in accordance with the invention;

35

Figure 11 is a sectioned view of a receiver module having a built-in bulbous tip of soft and compliant material in accordance with the invention;

Figure 12 is a sectioned view of a receiver module adapted to connect to a snap-on soft tip in accordance with the invention;

5 Figure 13 is a sectioned view of a receiver module adapted to connect to a sealing tip via a threaded screw in accordance with the invention;

Figure 14 is a sectioned view of a receiver module having an articulated sealing tip in accordance with the invention;

10 Figure 15 is a side view of a receiver module having multiple grooves and sealing rings in accordance with the invention;

Figures 16a-16e are side views of alternative sealing rings for use with the receiver modules of Figures 15 and 17 in accordance with the invention;

15 Figure 17 is a side view of a receiver module having a single groove in accordance with the invention;

20 Figure 18 is a sectioned view of a receiver module having a sleeve seal in accordance with the invention;

Figure 19 is a sectioned view of an adjustable shaft connector using hollow screws and a screw sleeve in accordance with the invention;

25 Figure 20 is a sectioned view of an adjustable connector using a telescopic shaft having a compression nut in accordance with the invention;

Figure 21 is a perspective view of a compressible cylinder around a connector in accordance with the invention;

30 Figure 22 is a partially sectioned, perspective view of a compressible cylinder having a cloth surface in accordance with the invention;

35 Figure 23 is a coronal view of a completely-in-the-ear-canal configuration of an articulated hearing device in accordance with the invention;

Figure 24 shows single ball-joint articulation with a short connector in accordance with the invention;

Figure 25 shows single ball-joint articulation with a long connector in accordance with the invention;

5 Figure 26 shows double articulation with a tapered boot and a ball joint in accordance with the invention;

Figure 27 shows a continuous articulation connector in accordance with the invention;

10 Figure 28 shows a spring coil connector in accordance with the invention;

Figure 29 shows a modular articulated hearing device having detachable parts in accordance with the invention;

15 Figure 30 shows an articulated hearing device microphone adapted to receive direct acoustic input from a virtual electroacoustic audiometer in accordance with the invention;

20 Figure 31 shows an articulated intra-canal prosthesis in accordance with the invention; and

Figure 32 is a partially exploded view showing sizers for an articulated hearing aid in accordance with the invention.

25

DETAILED DESCRIPTION OF THE INVENTION

30 The hearing device described herein is used for hearing enhancement and auditory rehabilitation of hearing impaired individuals. The hearing device is also adapted for use as an Intra-Canal-Prosthesis (ICP) in conjunction with a Virtual Electroacoustic Audiometer (VEA), both of which are described in U.S. patent application serial nos. 08/292,072, 08/292,067 and 08/292,073, all of which were filed on 17 August 1994.

35 Figs. 3 and 4 show coronal and transverse views, respectively, of the major components of the preferred embodiment of the herein disclosed hearing device 10 inserted in the right ear canal 11.

The main module 12 includes all of the typical components found in a hearing devices, except for the receiver. These components include a housing 13, a battery compartment 15, a battery 16, a relatively large vent 18, a signal processor circuit 17 such as the miniature high fidelity non-programmable hybrid ER101-28D manufactured by Etymotic Research of Elk Grove Village, Illinois, and a low noise microphone 14 such as the EM4068 manufactured by Knowles Electronics of Itasca, Illinois.

The receiver module 40 includes a receiver 41, a rigid housing 42, and an external housing made of a soft and malleable material 43. The receiver 40 is deeply positioned within the ear canal, preferably in the bony portion 29 of the canal. The receiver module acoustically seals the device in the bony area as shown in Figs. 3 and 4. A small vent 44 within the receiver 40 acts primarily as a pressure relief vent.

A connector 50 contains electrical wires 51 that carry electrical signals representing processed acoustic signals 19. The connector in the preferred embodiment of the invention contains hollow screw shafts 52 that are articulated with the main module 12 via a tapered boot 54, and with the receiver module 40 via another tapered boot 55. The length of the connector shaft is adjustable via the adjusting screw sleeve 53 to accommodate variability in ear canal lengths.

Separation of the receiver from the main module, and the receiver's articulation with respect to the main module, allows the receiver to have at least two degrees of freedom in movement. This freedom of movement allows essentially independent movement of the receiver module with respect to the main module, and *vice versa*. The articulation facilitates deep device insertion and removal, particularly in narrow and tortuous ear canals. The articulation is also important for accommodating various normal and abnormal ear canal deformations.

Fig. 5 shows the articulated device as it responds to a particular mandibular pressure from the condyle 33. This pressure is represented by a vector 60 having a radial component 61 and an axial component 62. Ear canal deformations that are due to direct mandibular pressure are shown by the dashed line 63. The articulated hearing device, particularly at the main module 12 and at the connector 50, shifts in response to the mandibular

pressure and causes a secondary ear canal deformation, as shown by the dotted line 65.

5 Radial pressure generally has minimal effect on the device because the diameter of the connector 50 is smaller than the diameter of the ear canal, as shown in the figure. Axial pressure which is generally smaller, causes the main 12 module, and subsequently the connector 50, to move and rotate in the direction of the arrow 64, as is shown in the figure. These device movements have minimal effect on the articulated receiver module 40, thus
10 allowing the receiver module to maintain an acoustic seal with the ear canal, such that the device is comfortable to wear during various mandibular motions. This combination of comfort and continuous acoustic sealing during mandibular motion is not possible with conventional hearing aid designs that employ contiguous housings and non-articulated parts.

15

Another advantage of the invention is improved retention of the device within the ear canal. This is due to the essentially independent movement of device parts in response to various mandibular motions.

20 By positioning the receiver in the articulated receiver module, instead of in the main module as in conventional designs, substantial reduction in the size of the main module is realized. Typical receivers for use with this invention include the ES series manufactured by Knowles Electronics which are 7.5 mm. long, 3.58 mm high, and 3 mm wide. The OV series receiver,
25 also manufactured by Knowles, is slightly larger but its oval shape better conforms to the natural shape of a typical ear canal. The size reduction due to repositioning the receiver away from the main module is significant because it allows a smaller main module to fit deeper in the medial concha area 20, which is generally more uniform than the lateral concha area 34.

30

Single or multiple controls 9, e.g. miniature trimmers (see Figs. 6-8) are typically needed for the non-programmable hearing device and are typically positioned on the face-plate side 56 of the hearing device. For programmable hearing devices, a programmable signal processor circuit
35 17, such as the ER-102, also manufactured by Etymotic Research, may be used. This arrangement requires a miniature electrical connector (not shown) on the face plate, such as the CS44-01 manufactured by Microtronic of Roskilde, Denmark.

Other variations of component distribution within the hearing device are possible without departing from the principles of the invention. For example, many receivers, such as the ES series mentioned above, contain an integrated electronic circuit that is used for signal amplification. It is likely
5 that in the future additional circuits or even the entire signal processing circuit may be fully integrated within the receiver.

Figs. 6-8 show detailed dimensions of a pediatric, adult, and large size main module housing, respectively, in accordance with various embodiments of
10 the invention. The size of the main module in the example embodiments shown in Figs. 6-8 is largely determined by the battery size. A pediatric-size device, designed primarily for children, uses battery sizes 5A and 10A; the adult-size main module uses 10A or 312A battery; and a large-size main
15 module, designed for large ears or for individuals having severely impaired hearing, requires larger batteries of higher energy capacity, such as battery sizes 312A and 13.

The main module contains a relatively large vent 18 that presents minimal impedance to own-sounds, versus the higher impedance smaller vent 44 of
20 the receiver module 40. This venting arrangement prevents leakage of own-sounds into the tympanic membrane. The large vent of the main module, or venting via loosely inserted device, also improves air circulation to the tissue in the cartilaginous area. The unique design of the articulated hearing
25 device herein disclosed provides a highly vented device, without such concerns for oscillatory feedback as are common to conventional hearing devices having a contiguous housing.

Figs. 6-8 show typical dimensions of housings in the preferred embodiment for pediatric (Figs. 6a and 6b), adult (Figs. 7a and 7b), and large (Figs. 8a
30 and 8b) main modules. These designs were developed from averaged ear canal impressions taken of twelve adults and two children, including six pairs of complete impressions taken from adult cadavers. The principal criteria for the main module design is that it should fit deeply and comfortably within the medial concha of most individuals, although an exact match of the
35 main module to the shape of each ear canal is not required.

Figs. 9a and 9b show the preferred articulation angle, range of articulation, and range of dimensions for the preferred embodiment of the invention in the coronal (Fig. 9a) and transverse (Fig. 9b) views. The diameters of the

main module are approximately 15 mm and 9.5 mm in the coronal and transverse planes, respectively. The articulation of the main module with the connector is nominally at angles of about 170° and about 135° in the coronal and transverse planes, respectively, with an additional range of articulation of approximately 30°. The length of the connector is approximately 5 mm +/-3 mm. The receiver articulates with the connector approximately with nominal angles of about 190° and about 225° in the coronal and transverse planes, respectively. An additional range of articulation of approximately 30° is preferred. The length of the receiver module is approximately 6.5 mm +/-2 mm with diameters of 4.5 mm and 3.5 mm in the coronal plane and transverse plane, respectively.

The invention incorporates several design options that reduce or eliminate various causes of oscillatory feedback, including:

15

1. Reduction of Feedback Due To Independent Motion of Main Modules. As described above, the independent motion of the articulated hearing device modules prevents oscillatory feedback due to acoustic leakage conventionally caused by various ear canal deformations. This oscillatory feedback occurs when the microphone of the hearing device receives some of the acoustic energy that is produced by the receiver.

20

2. Reduction of Feedback Due To External Acoustic Leakage. External leakage due to imprecise device fit also represents a common cause of oscillatory feedback. In addition to the basic principles of the articulated hearing device relating to feedback reduction, the following represent additional features of the invention that reduce external acoustic leakage feedback:

25

a. A receiver module 40 having a built-in compliant sealing housing 43, as shown in Fig. 10, made of a soft material such as medical grade silicone. The pressure vent 44 may also be used for inserting a probe tube 45 into the ear canal during real-ear and VEA measurements.

30

b. A receiver module 40 having a built-in sealing bulbous tip 70, as shown in Fig. 11, also made of a soft compliant material such as medical grade silicone. A semi-rigid tubing 71 prevents the tip 70 from fully collapsing and occluding the sound from the receiver port 72.

35

c. A receiver module 40, as shown in Fig. 12, that is adapted to connect to a snap-on sealing tip 80, which is made of a soft material such as silicone or foam. The connection to the receiver port 72 is made via snap-on connectors 81. Orientation of the sealing tip 80 with the receiver 41 for probe
5 tube insertion is assured via an alignment insert 82.

d. A receiver module 40, as shown in Fig. 13, that is adapted to connect via threaded connections 91, 92 to a sealing tip 90, which is made of a soft material such as silicone or foam.

10

e. A receiver module 40, as shown in Fig. 14, that is adapted to connect to an articulated tip 100, which is made of a soft material such as silicone or foam. The articulation is provided via a ball joint 101 and a ball socket 102.

15 f. A receiver module 40, as shown in Figs. 15 and 17, that is adapted to connect to multiple or single sealing rings 110, respectively, on multiple or single grooves 111, respectively, on the surface of a receiver 40. The rings are made of a soft compliant material such as silicone or foam. The rings 110a-110e may have various diameters and/or profiles as desired (see, for
20 example Figs. 16a-16e).

g. A receiver module 40, as shown in Fig. 18, having a sleeve seal 190 that is made of a soft compliant material such as silicone or foam.

25 The separable sealing parts, described above, are preferably washable or disposable.

3. Reduction of Feedback Due To Internal Acoustic Leakage. Another type of oscillatory feedback is caused by acoustic leakage that is conducted
30 internally from the receiver to the microphone of conventional hearing devices. The invention substantially reduces this type of feedback because the receiver is completely encapsulated and is essentially isolated from the internal components of the main module, particularly the microphone.

35 4. Reduction of Feedback Due To Shell Vibrations. Another type of feedback that is substantially reduced by the invention is feedback caused by receiver vibration that is conducted to the microphone via the contiguous rigid shell used in conventional hearing aids. The articulated hearing device

consists of separated parts, therefore, there is no contiguous surface to conduct receiver vibration.

5. Reduction of Feedback Due To Piston Action of High Sound Pressures.

- 5 This type of feedback, common in hearing devices having very high acoustic gains in excess of 50 dB, is referred to as the piston action feedback. Such feedback is caused by high sound pressure levels that are produced in the ear canal that cause the entire hearing device to vibrate. Sound waves are externally generated from the vibrating face-plate of the hearing device.
- 10 When reflective surfaces such as telephone receivers or hands are placed near the vibrating hearing device, these sound waves can bounce back into the microphone of the hearing device and cause oscillatory feedback. The invention substantially decouples the movements of the receiver from the main module, thus reducing piston action feedback common to conventional
- 15 hearing aids that have a contiguous housing. Furthermore, the viscoelastic material incorporated into the connector, as is described in greater detail below, further reduces piston action feedback.

- 20 The receiver module 40 is preferably inserted in the bony region 29 of the ear canal to maximize the electroacoustic benefits associated with close receiver proximity to the tympanic membrane. For persons having extreme tissue sensitivity, the receiver may be placed in the deeper portion of the cartilaginous region 23 of the ear canal, preferably at the junction of the cartilaginous-bony areas. The depth of receiver insertion may be adjusted
- 25 using an adjustable length connector. The receiver module 40 may also be incrementally positioned deeper in the ear canal, via the adjustable connector, as the individual gradually adapts to the receiver.

- 30 An example of an adjustable connector 50 is a turnbuckle shaft having an adjusting screw sleeve 53, as is shown in Fig. 19. The threads of one of the shafts are reversed to allow for connector 50 expansion or contraction via the rotation of the adjusting screw sleeve 53, which also has reversed threads on one of its sides. A sheath 112 encapsulates the connector to protect against dirt and physiological byproducts, *e.g.* sweat and cerumen.

- 35 Another variation of the adjustable connector is the telescopic shaft shown in Fig. 20, where a compression nut 46 and a compression ring 59 are used to secure a long shaft 58 to a short screw shaft 57, according to the desired length of the connector. Other methods of connector adjustment are

possible and will be obvious to persons skilled in the art of miniature mechanics.

5 In the invention, the connector 50 diameter is less than the diameter of the ear canal in the cartilaginous area to accommodate various ear canal deformations. The connector may also incorporate a compressible cylinder 120, as shown in Fig. 21 to reduce further the possibility of external acoustic leakage that causes oscillatory feedback. The cylinder is preferably disposable and made of a foam material, such as E.A.R., manufactured by
10 Cobot Safety Corporation of Indianapolis, Indiana, or Comply, manufactured by Hearing Components, Inc. of Maplewood, Minnesota. In addition to acoustic sealing in the cartilaginous area, the cylinder facilitates cerumen collection because it is positioned in the primary area of cerumen production. This arrangement prevents cerumen accumulation in the ear
15 canal, a problem common to many hearing aid users, particularly the elderly.

Another variation of the cylinder around the connector, shown in Fig. 22, incorporates a cloth surface 121 on the cylinder 120 to facilitate cerumen
20 collection. The cloth is preferably made of a soft, non-abrasive, biocompatible material such as cotton.

The main module 12 may also be inserted deeper in the ear canal beyond the canal aperture 24 and within the cartilaginous area 28, as is shown in
25 Fig. 23. In this completely-in-the-canal (CIC) configuration, the main module is preferably loosely fitted in the cartilaginous area of the ear canal. An extraction line 130, typically made of nylon, facilitates the removal of the articulated device. The CIC configuration is suitable for persons having relatively good manual dexterity, who prefer a highly inconspicuous hearing
30 device having maximum cosmetic appeal. The deep-concha configuration, shown in Figs. 3 and 4, which is also inconspicuous, is especially suitable for persons having relatively poor manual dexterity.

Both the CIC and the deep concha hearing device configurations, Figs. 23
35 and 3, respectively, are designed to take advantage of the natural acoustic features of the concha 34 and pinna 35 areas of the ear. These benefits include selective frequency amplification and sound localization.

The articulation for the hearing device of the invention is achieved by a variety of means. Fig. 24 shows a single articulation between the main module 12 and the receiver module 40, with a short connector 50. The articulation consists of a ball-joint mechanism having a ball 140 and a ball
5 socket 141.

Fig. 25 shows a single articulation at the receiver module 40 with a long connector 50. The ball-joint articulation consists of a ball 140 and a ball
10 socket 141.

Fig. 26 shows double articulations at each end of the connector 50. The articulation consists of a ball 140 and a ball socket 141 at the receiver module end of the connector, and a tapered boot 54 at the main module end of the connector. The boot 54, or the connector in general, may incorporate
15 a viscoelastic material to isolate mechanical vibration among the device parts.

The articulation may also be obtained via a flexible connector 40, as is shown in Fig. 27. The flexible shaft shown provides continuous articulation
20 across the connector part. The grooves 114 may be patterned, as shown, to provide more articulation at receiver module 40 and main module 12 ends of the connector, as compared with a relatively more rigid central part of the connector 50.

The articulation may be also obtained via a spring coil 113 connector, as is shown in Fig. 28. The spring coil connector is preferably made of stainless steel, where the outside coil diameter is in the range of about 1.5 mm to about 3 mm, and where wire diameter is in the range of about 0.15 mm to about 0.3 mm. The pitch of the coil is preferably tight, with a tensile strength
30 in the range of about 250 to about 340 pounds per square inch.

Other embodiments of the invention that provide articulation at the receiver module, main module, or connector are possible and will be obvious to persons skilled in the art of micro-mechanics and materials.

35 The preferred embodiment of the invention is a universal hearing device that does not require custom manufacturing or the taking of individual ear canal impressions. The main module is designed to be loosely fitted, and generally fills the relatively compliant outer portions of the ear canal. The

receiver module provides wearing comfort by articulating when it is inserted and removed, and during various ear canal deformations. The receiver module seals individual ear canals of various sizes and shapes via its malleable housing, or via one of the various acoustic seals discussed
5 above. The sealing tips are preferably assorted to allow for customization of the device at the dispensing site. The assorted sizes of main modules also allow for a broad physical fitting range, including children, adults, persons having large ears, and persons who are severely hearing impaired.

10 In another embodiment of the invention, the device may be custom manufactured according to an ear impression or any other method where the details of the ear canal can be measured or described. Alternatively, the device may be partially custom manufactured. For example, the receiver
15 module or the main module may be fabricated according to a partial impression of the ear canal representing the part to be customized.

In another embodiment of the invention, the parts of the hearing device are modular, detachable, and interchangeable for in-office customization and assembly. Fig. 29 shows a modular hearing aid having an articulated
20 receiver module and a connector that is detachable from a three-pin connector 150 via a coupler screw 151 and a coupling nut 152. Other detachable areas, not shown, may include the center of the connector, the receiver-connector junction, and other areas that will be obvious to persons skilled in the art.

25 The microphone of the articulated hearing device may be adapted to receive direct acoustic signals from a virtual electroacoustic audiometer, such as disclosed in U.S. patent application serial nos. 08/292,072 and 08/292,073, referenced above. As shown in Fig. 30, the microphone 14 is connected to a
30 microphone port 162 that connects to a receiver 161 via an acoustic coupler 160. The receiver 161 is connected to the virtual electroacoustic audiometer (not shown) which presents acoustic signals directly to the articulated hearing device for aided hearing evaluation. A probe tube 164 is inserted via a main module vent 18 and a receiver vent 44, as is shown in Fig. 30.
35 The probe tube is used to measure the acoustic response in the ear canal near the tympanic membrane from signals generated via the receiver 40.

An intra-canal prosthesis (ICP), disclosed in above referenced U.S. patent application serial no. 08/292,067, is adapted for articulation, as is shown in

Fig. 31. The articulated ICP 170 is provided in the form of an articulated hearing device having a main module 172 that only contains an electrical connector 171 which routes electrical signals directly from a virtual electroacoustic audiometer (not shown), via a connector 175, to ICP receiver 173. A probe tube 164 is inserted in the ICP vent 174. The ICP probe tube 164 is used to measure the acoustic response in the ear canal near the tympanic membrane from acoustic signals generated via the ICP receiver 173. The ICP is generally used to perform intra-canal diagnostics and hearing aid simulation as disclosed in above referenced U.S. patent application serial nos. 08/292,067 and 08/292,073. In this embodiment of the invention, the ICP is adapted to perform unaided, simulated aided hearing evaluation in accordance with virtual electroacoustic audiometry.

Sizers that represent the articulated hearing device in terms of physical characteristics, shown in Fig. 32, can be used to predetermine the optimal physical configuration of the hearing device for an individual prior to final device insertion. Sizers include main module sizers 180, connector sizers 181, receiver sizers 182, and seal tip sizers 183. The sizer parts are removably attached, preferably using snap-on connections 184, as shown. The main module sizer 180 may be directly attached to the receiver sizer 182 to represent hearing devices that have a very short connector. Other sizer shapes and articulation methods, representing the articulated hearing device of the present invention are possible and can be implemented by persons skilled in the art.

Although the invention is described herein with reference to the preferred embodiment, one skilled in the art will readily appreciate that other elements, materials, and applications may be substituted for those set forth herein without departing from the spirit and scope of the present invention. Accordingly, the invention should only be limited by the Claims included below.

CLAIMS

1. A hearing device, comprising:
 - 5 a main module adapted to contain any of a microphone, a battery, device controls, and a signal processing circuit;
 - a receiver module adapted to contain a receiver; and
 - a connector adapted to provide an electrical connection between said main module and said receiver module;
- 10 wherein at least two of said main module, receiver module, and connector are articulated, one relative to the other, to facilitate deep placement of said receiver module in a patient's ear canal, and to permit independent movement of any of said main module, said receiver module, and said connector in response to ear canal deformation.
- 15
2. The hearing device of Claim 1, wherein said main module is positioned in a medial concha area of said ear canal just behind the tragus.
3. The hearing device of Claim 1, said main module further comprising:
 - 20 a face-plate positioned either flush with or beyond an ear canal aperture.
4. The hearing device of Claim 1, said main module further comprising:
 - 25 controls positioned on a main module face plate.
- 25
5. The hearing device of Claim 1, where main module controls are programmed into said main module.
6. The hearing device of Claim 1, wherein any or all of said main module, said receiver module, and said connector are manufactured in
 - 30 assorted, standard sizes.
7. The hearing device of Claim 1, wherein any or all of said main module, said receiver module, and said connector are custom
 - 35 manufactured.
8. The hearing device of Claim 1, said receiver module further comprising:
 - means for reducing oscillatory feedback.

9. The hearing device of Claim 8, said means for reducing oscillatory feedback further comprising:
a soft and compliant housing.
- 5
10. The hearing device of Claim 8, said means for reducing oscillatory feedback further comprising:
a soft and compliant bulbous ending.
- 10
11. The hearing device of Claim 8, wherein said means for reducing oscillatory feedback is made of any of a silicone material or a foam material.
12. The hearing device of Claim 8, wherein said means for reducing oscillatory feedback is either disposable, washable, or both.
- 15
13. The hearing device of Claim 8, said oscillatory feedback reduction means further comprising:
a snap-on seal tip.
- 20
14. The hearing device of Claim 8, said oscillatory feedback reduction means further comprising:
a threaded seal tip.
- 25
15. The hearing device of Claim 8, said oscillatory feedback reduction means further comprising:
a tip that is articulated with respect to said receiver module.
- 30
16. The hearing device of Claim 8, said oscillatory feedback reduction means further comprising:
at least one sealing ring.
- 35
17. The hearing device of Claim 8, said oscillatory feedback reduction means further comprising:
a removable sleeve.
18. The hearing device Claim 1, said connector further comprising:
a covering for reducing oscillatory feedback.

19. The hearing device of Claim 1, said connector further comprising:
a covering having an absorbent layer for cerumen collection.
20. The hearing device of Claim 1, wherein said articulation is achieved
5 by at least one of:
a single point of articulation between said main module and said receiver module;
a single point of articulation between said receiver module and said connector;
10 a dual point of articulation at each end of said connector; and
a flexible connector adapted to provide at least one point of articulation between said receiver module and said main module.
21. The hearing device of Claim 1, further comprising:
15 means adapted to provide said articulation, including at least one of:
a ball joint;
a flexible joint;
a tapered boot;
a flexible connector;
20 a flexible shaft having alternating grooves; and
a spring coil.
22. The hearing device of Claim 1, wherein said receiver module is adapted to be positioned in any one of:
25 the bony area of the ear canal; and
the deeper cartilaginous area of the ear canal.
23. The hearing device of Claim 1, wherein the diameter of said connector is less than the diameter of the patient's ear canal, and is thereby
30 adapted to accommodate canal deformation.
24. The hearing device of Claim 1, wherein said connector is adapted to be positioned in the cartilaginous area of the ear canal.
- 35 25. The hearing device of Claim 1, wherein said connector is adjustable to accommodate a variety of individual ear canal lengths, and to permit receiver placement at a selected depth in the ear canal.

26. The hearing device of Claim 1, further comprising:
means for adjusting the length of said connector length, said
adjusting means comprising at least one of:
a turnbuckle shaft ; and
5 a telescoping shaft.
27. The hearing device of Claim 1, further comprising:
a plurality of modular, differently dimensioned, detachable sizers, said
sizers being adapted to determine at least optimal hearing device size,
10 patient comfort, hearing device ear canal insertion depth tolerance, ease of
ear canal insertion and removal, appearance, and overall hearing device
physical characteristics.
28. The hearing device of Claim 1, said main module further comprising:
15 a large vent adapted to receive a probe tube.
29. The hearing device of Claim 1, said main module further comprising:
a large vent adapted to vent the patient's ear canal to thereby reduce
occlusion effect and improve air circulation.
20
30. The hearing device of Claim 1, said receiver module further
comprising:
a canal adapted to receive a probe tube.
- 25 31. The hearing device of Claim 1, said receiver module further
comprising:
a canal adapted to provide pressure relief.
32. The hearing device of Claim 1, said main module including a
30 microphone, wherein said microphone is adapted to receive direct acoustic
input from a receiver in accordance with virtual electroacoustic audiometry.
33. The hearing device of Claim 1, wherein said receiver module is
adapted for deep insertion into the patient's ear canal to minimize or
35 eliminate occlusion effects.
34. The hearing device of Claim 1, said connector further comprising:
means for reducing vibration-caused oscillatory feedback.

35. The hearing device of Claim 34, wherein said means for reducing vibration-caused oscillatory feedback are made of a viscoelastic material.

5 36. The hearing device of Claim 1, said connector further comprising:
means for reducing piston action caused oscillatory feedback.

37. The hearing device of Claim 36, wherein said means for reducing piston action caused oscillatory feedback are made of a viscoelastic material.

10

38. An intra-canal prosthesis (ICP), said ICP being adapted to perform unaided, simulated aided hearing evaluation in accordance with virtual electroacoustic audiometry, said ICP comprising:

15 a main module adapted to provide an electrical connection to a virtual
electroacoustic audiometer;

a receiver module adapted to contain a receiver; and

a connector adapted to provide an electrical connection between
said main module and said receiver module;

20 wherein at least two of said main module, receiver module, and
connector are articulated, one relative to the other, to facilitate deep
placement of said receiver module in a patient's ear canal, and to permit
independent movement of any of said main module, said receiver module,
and said connector in response to ear canal deformation.

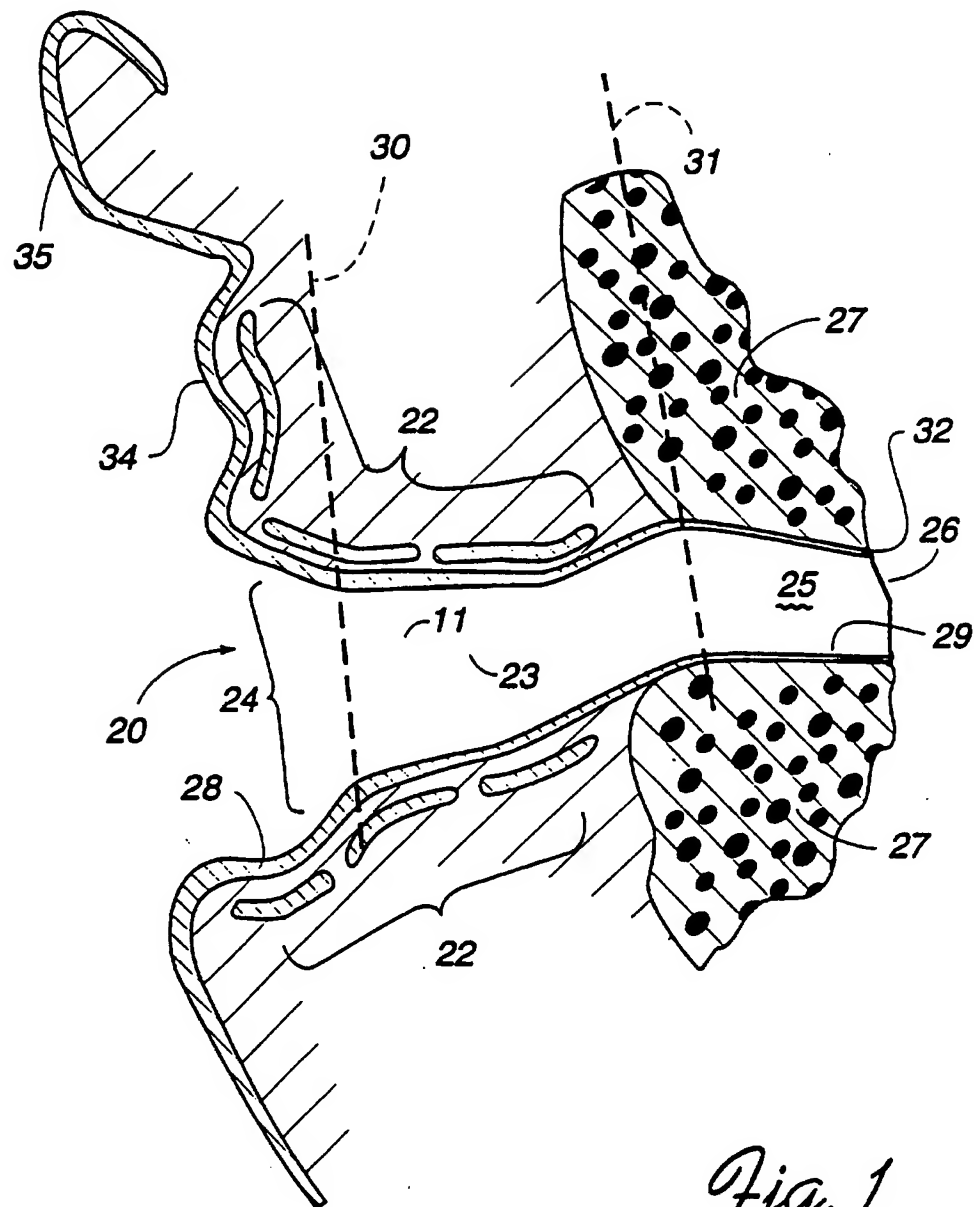


Fig. 1

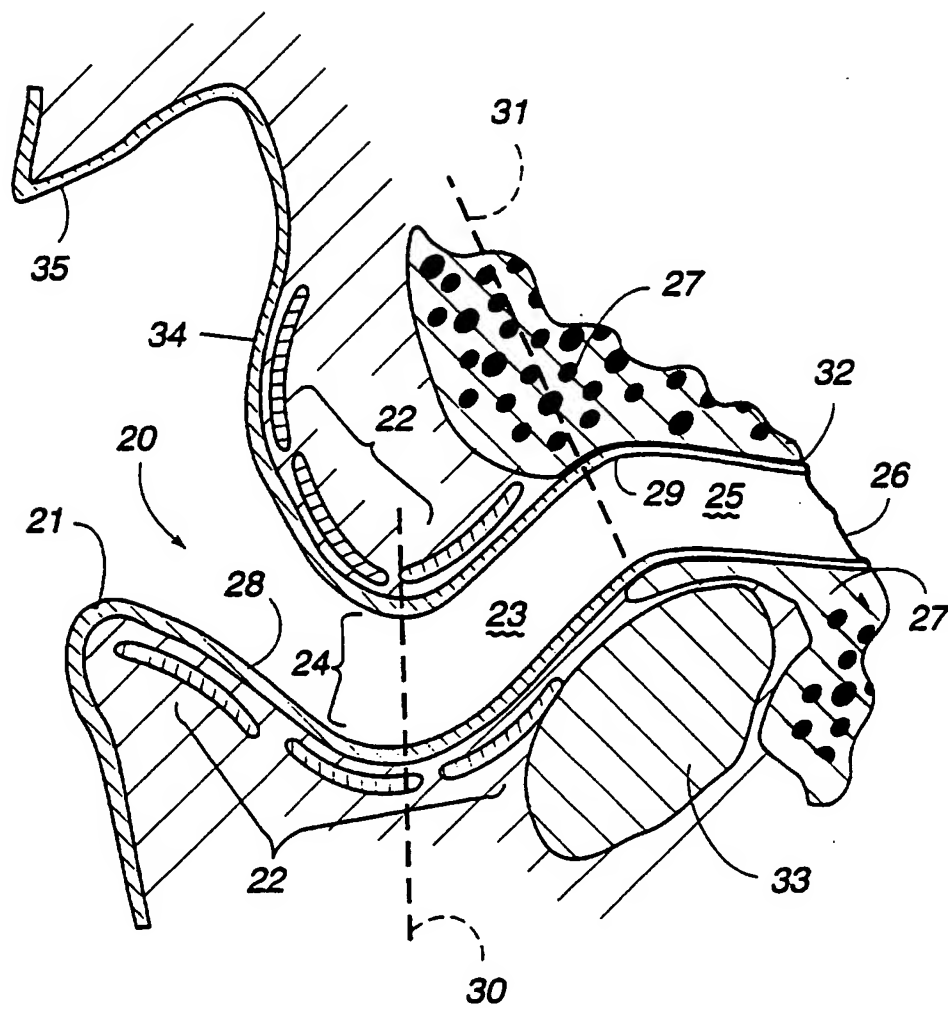


Fig. 2

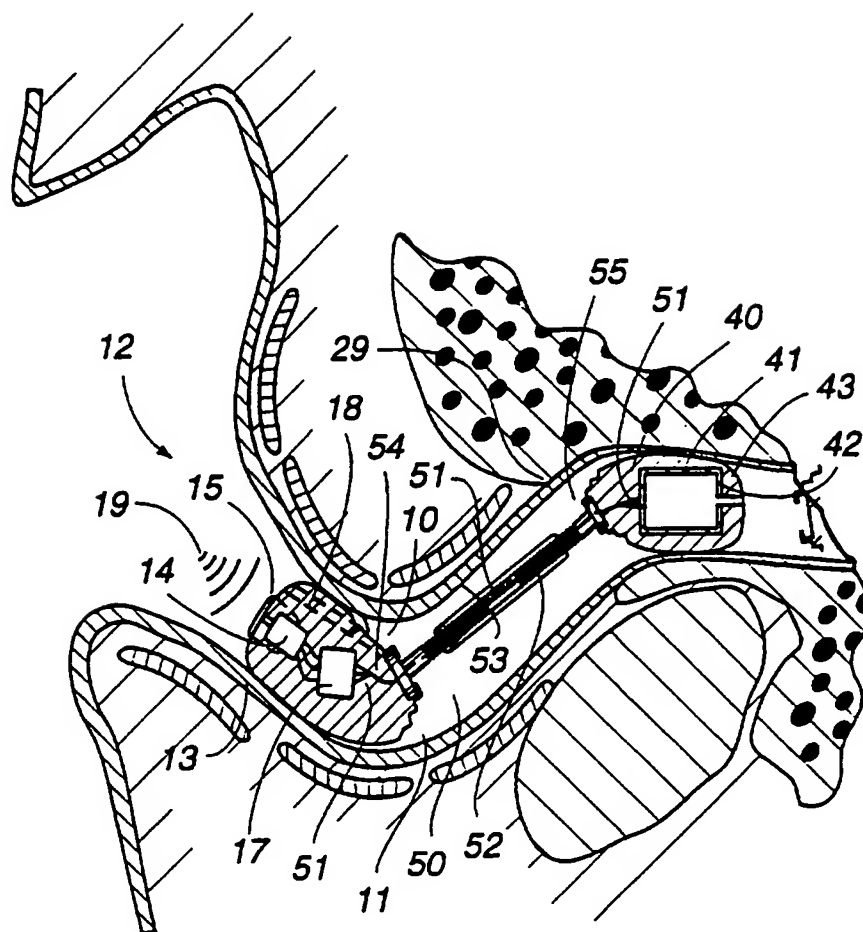
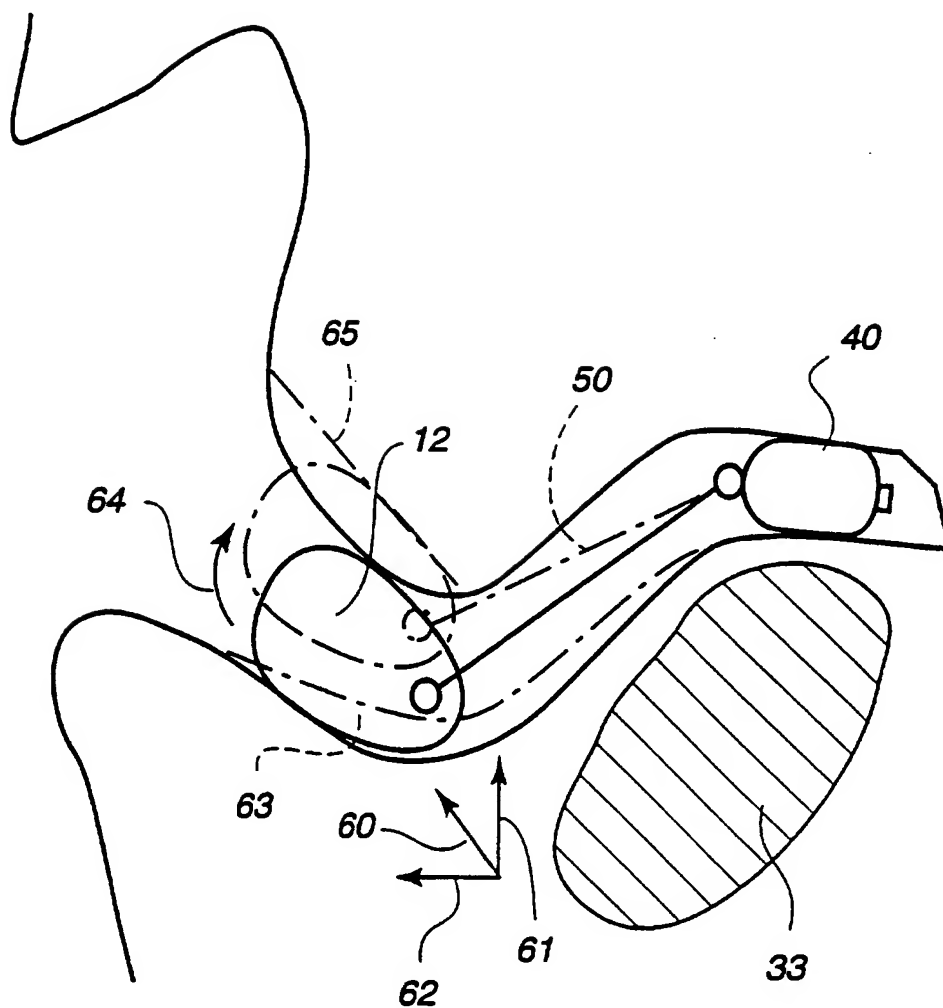


Fig. 4

*Fig. 5*

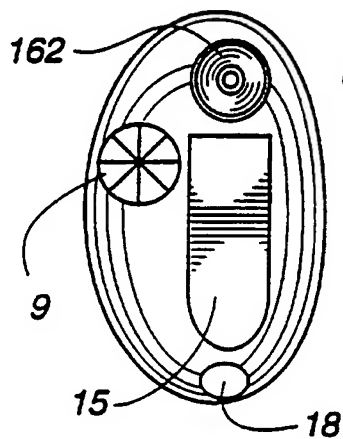


Fig. 6a

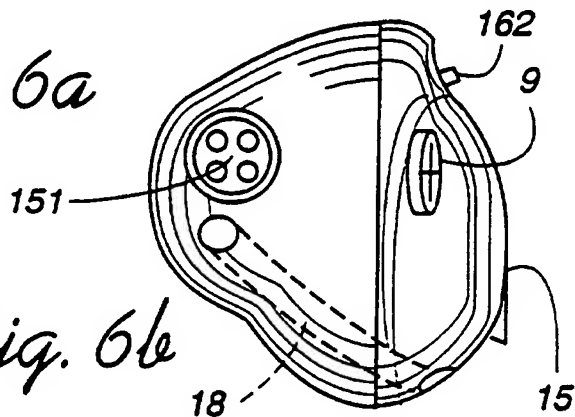


Fig. 6b

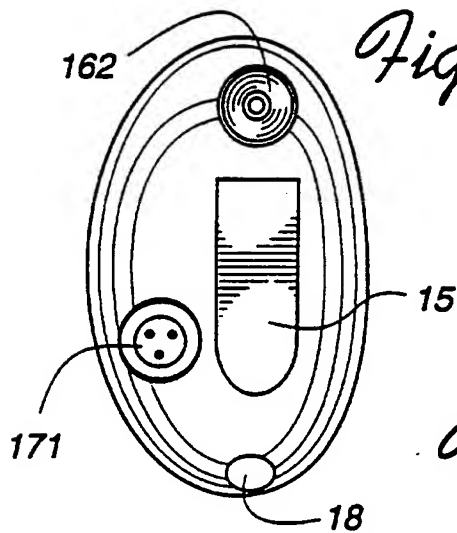


Fig. 7a

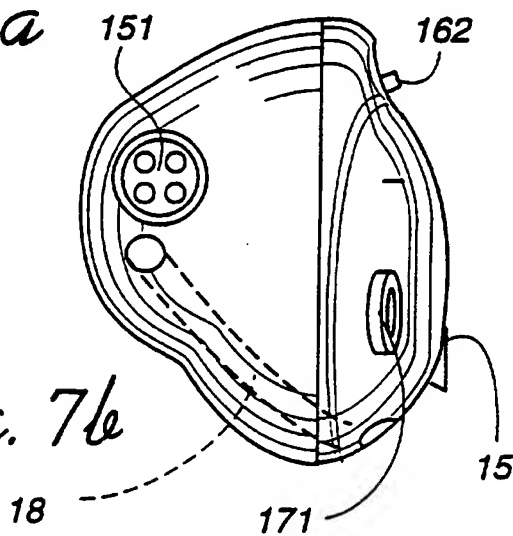


Fig. 7b

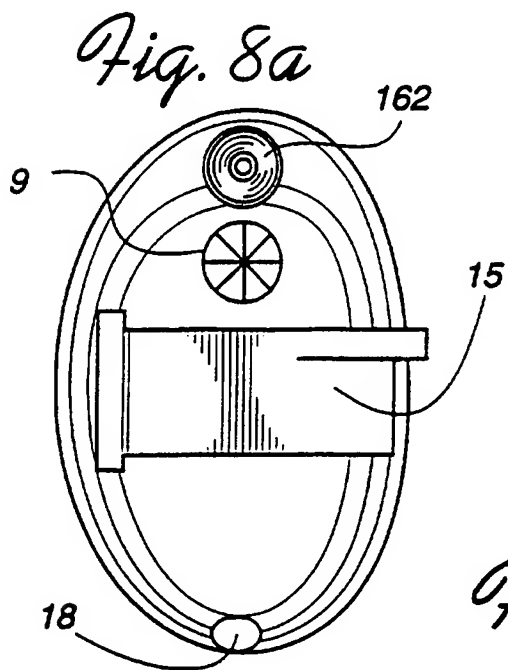


Fig. 8a

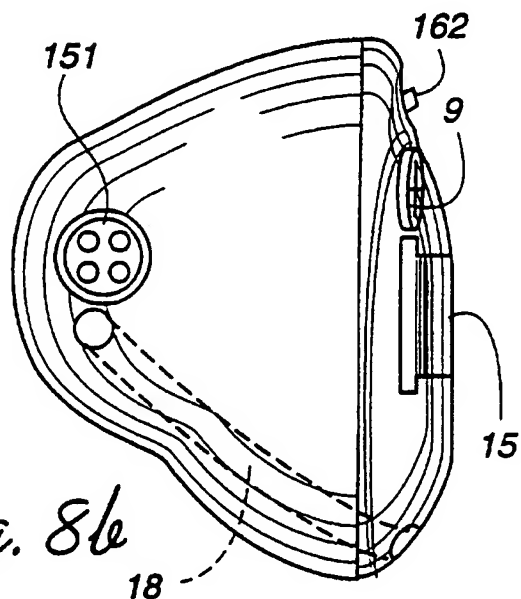


Fig. 8b

7/14

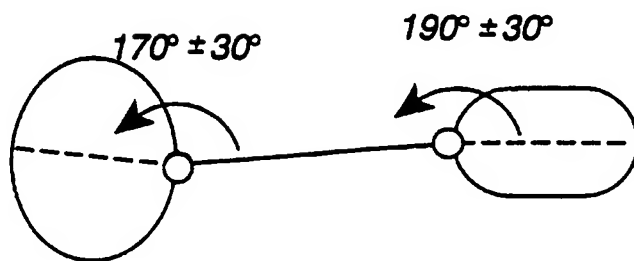


Fig. 9a

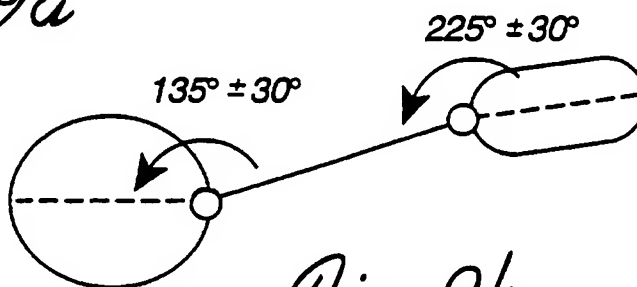


Fig. 9b

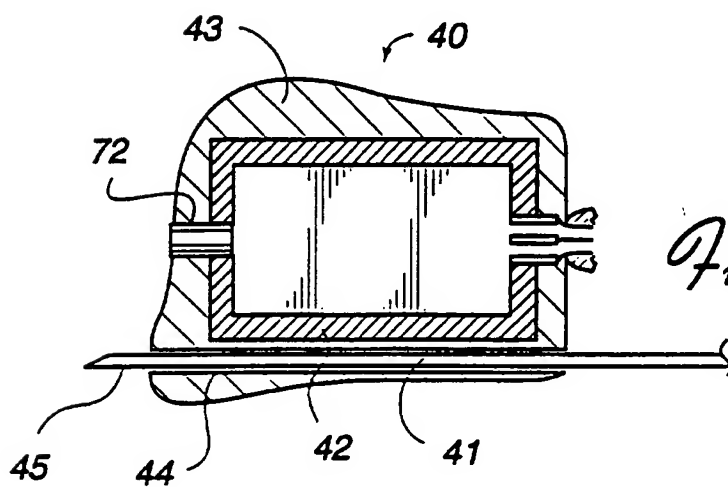


Fig. 10

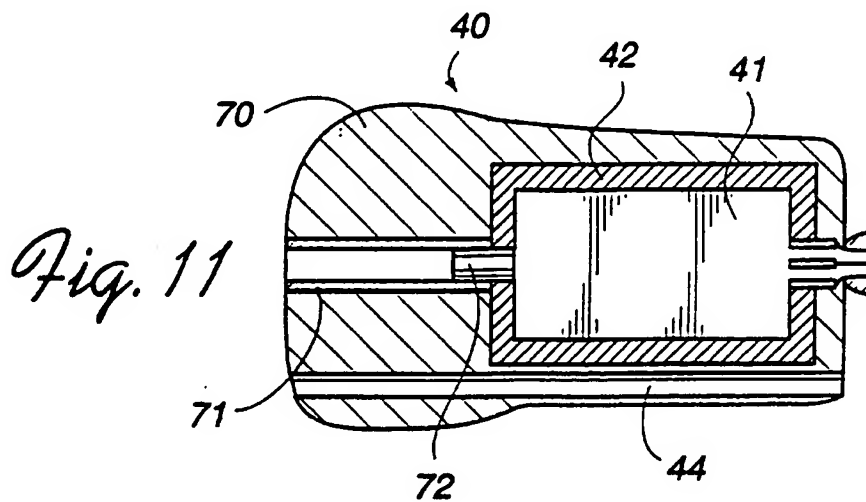
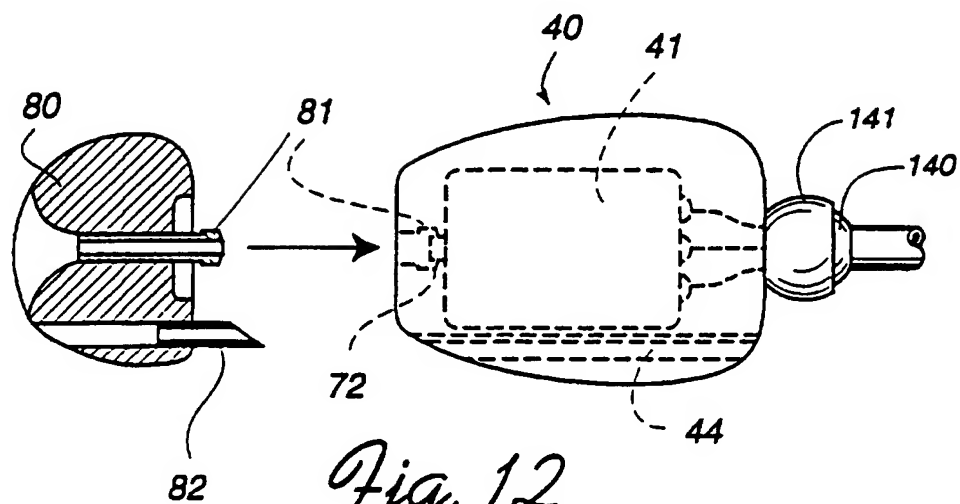
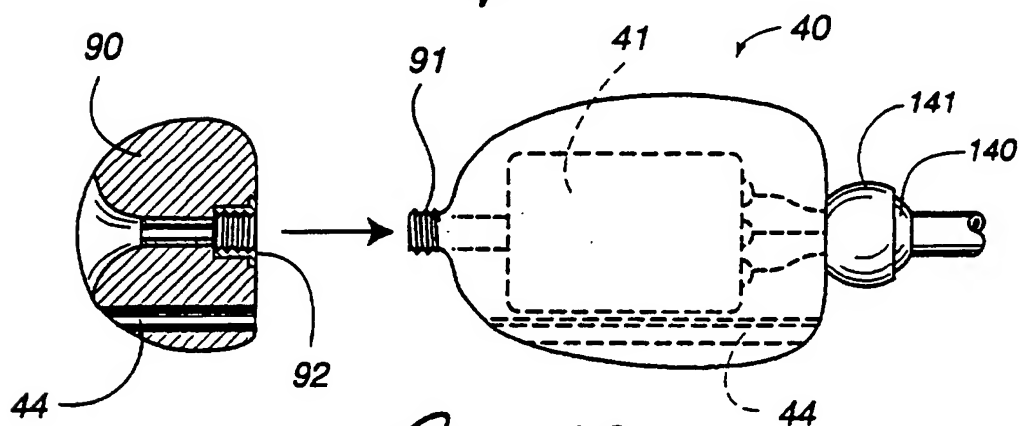
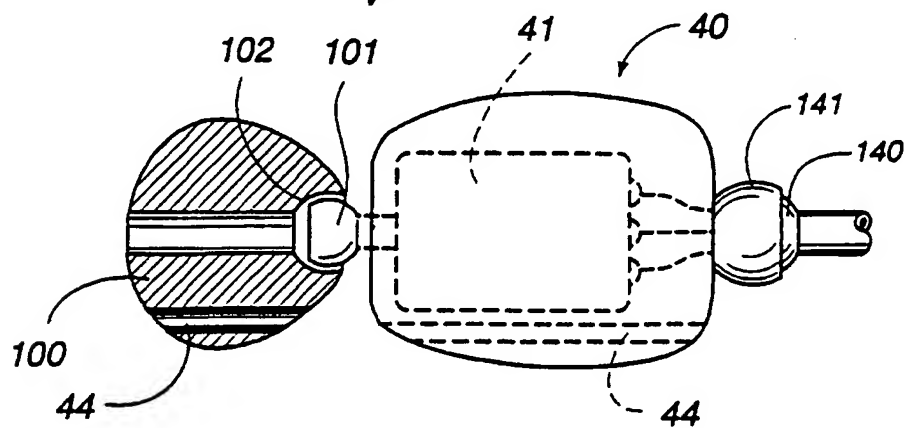


Fig. 11

*Fig. 12**Fig. 13**Fig. 14*

9/14

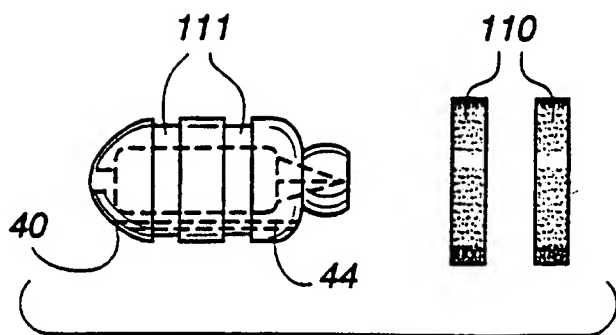


Fig. 15

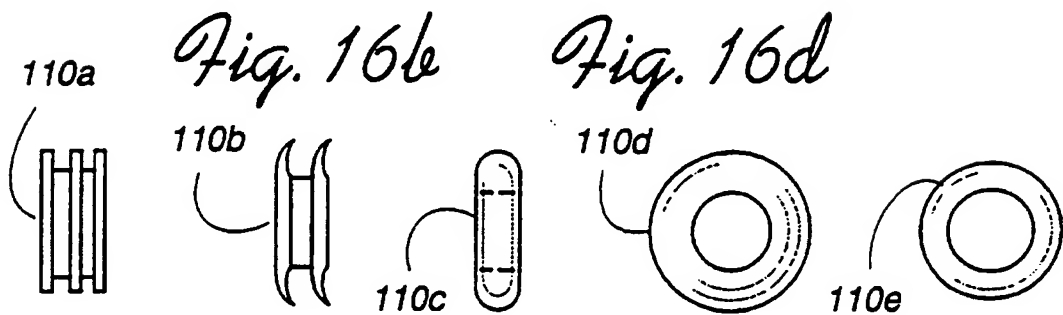


Fig. 16a

Fig. 16b

Fig. 16c

Fig. 16d

Fig. 16e

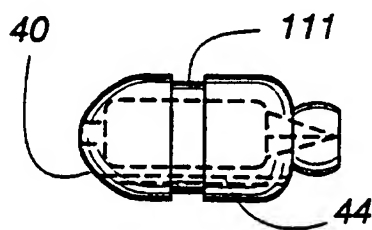


Fig. 17







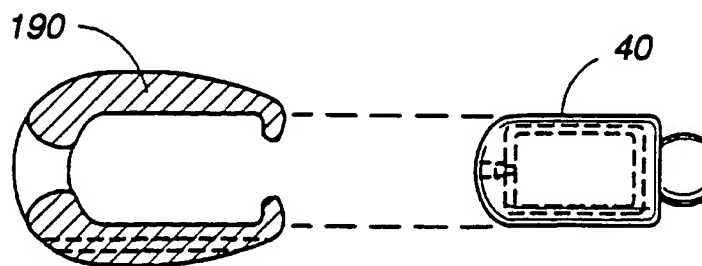


Fig. 18

10/14

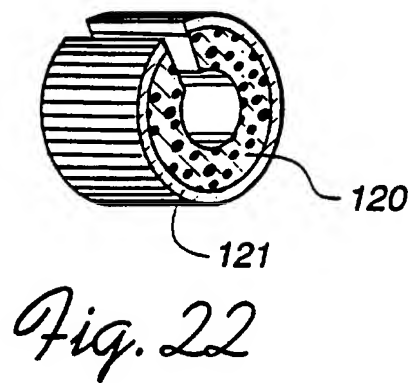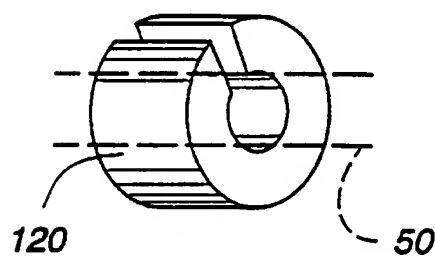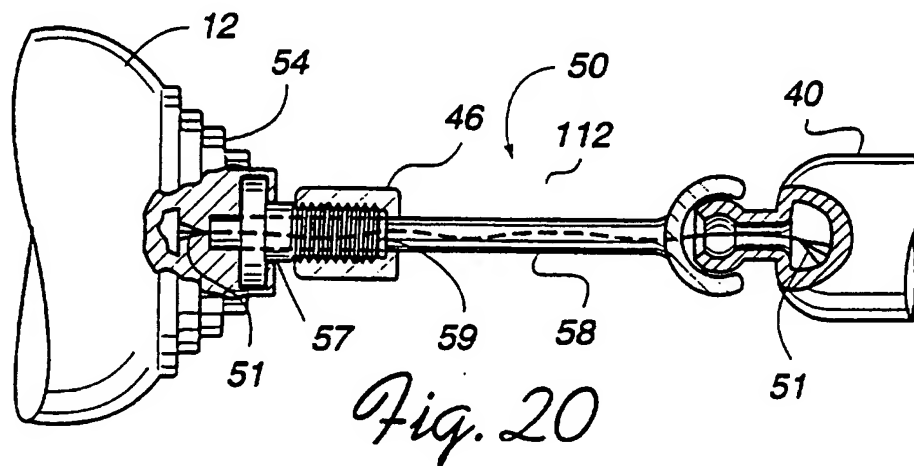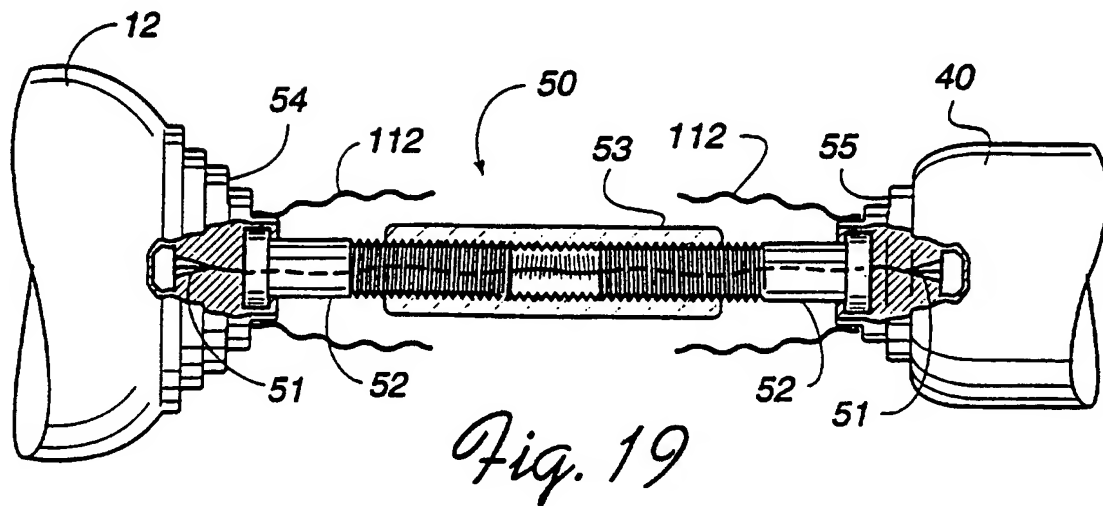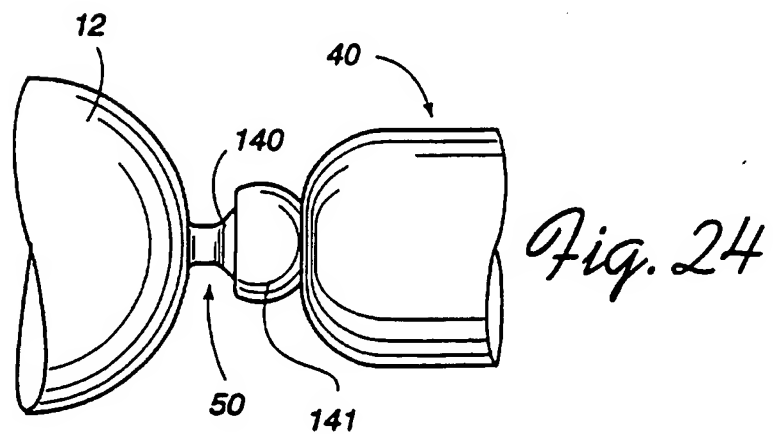

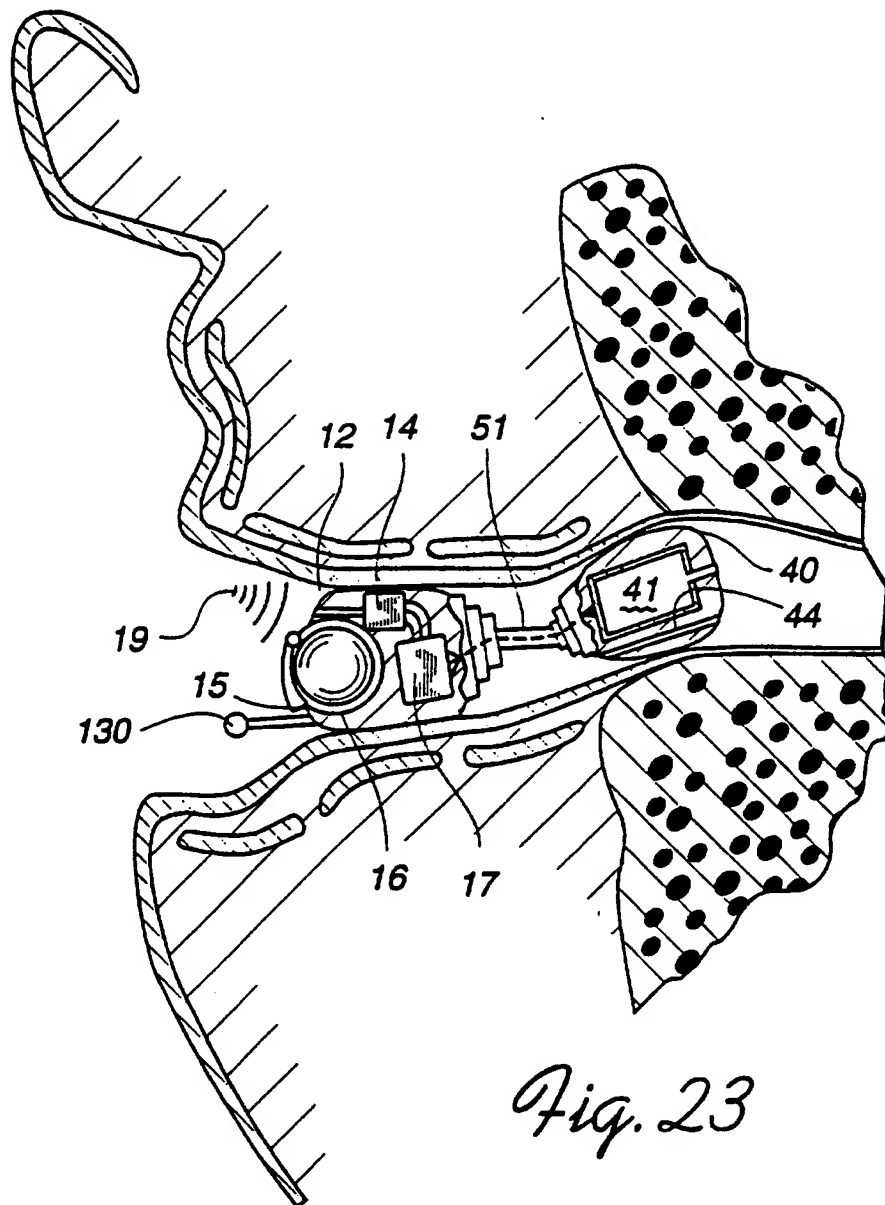

12/14

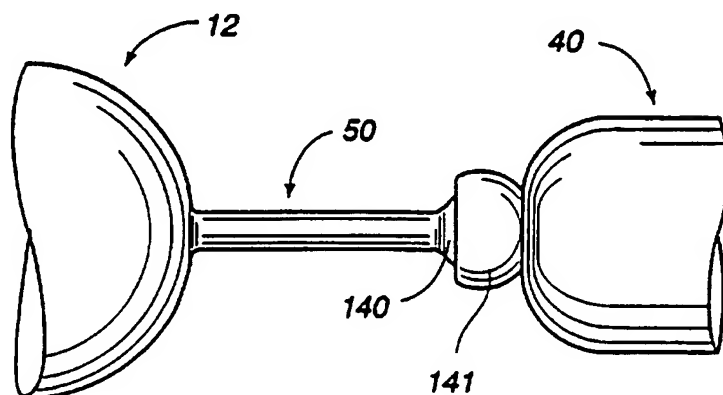


Fig. 25

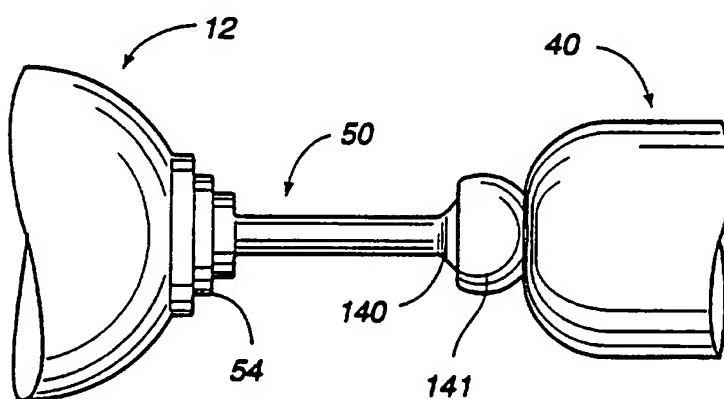


Fig. 26

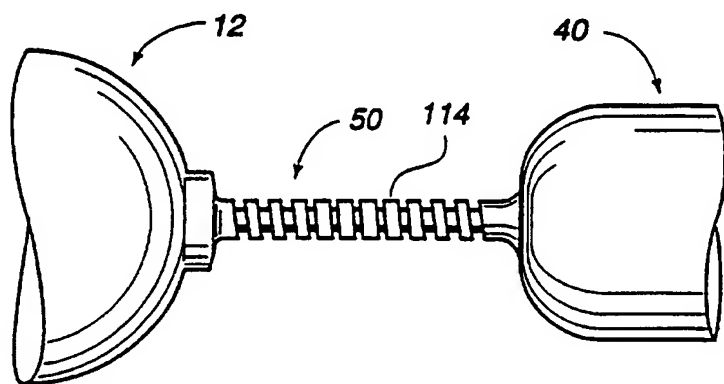


Fig. 27

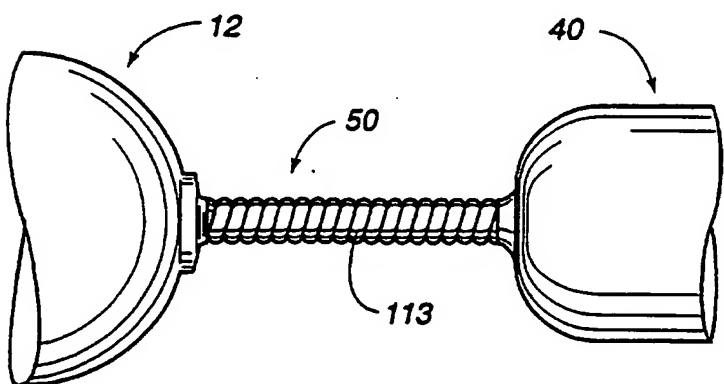
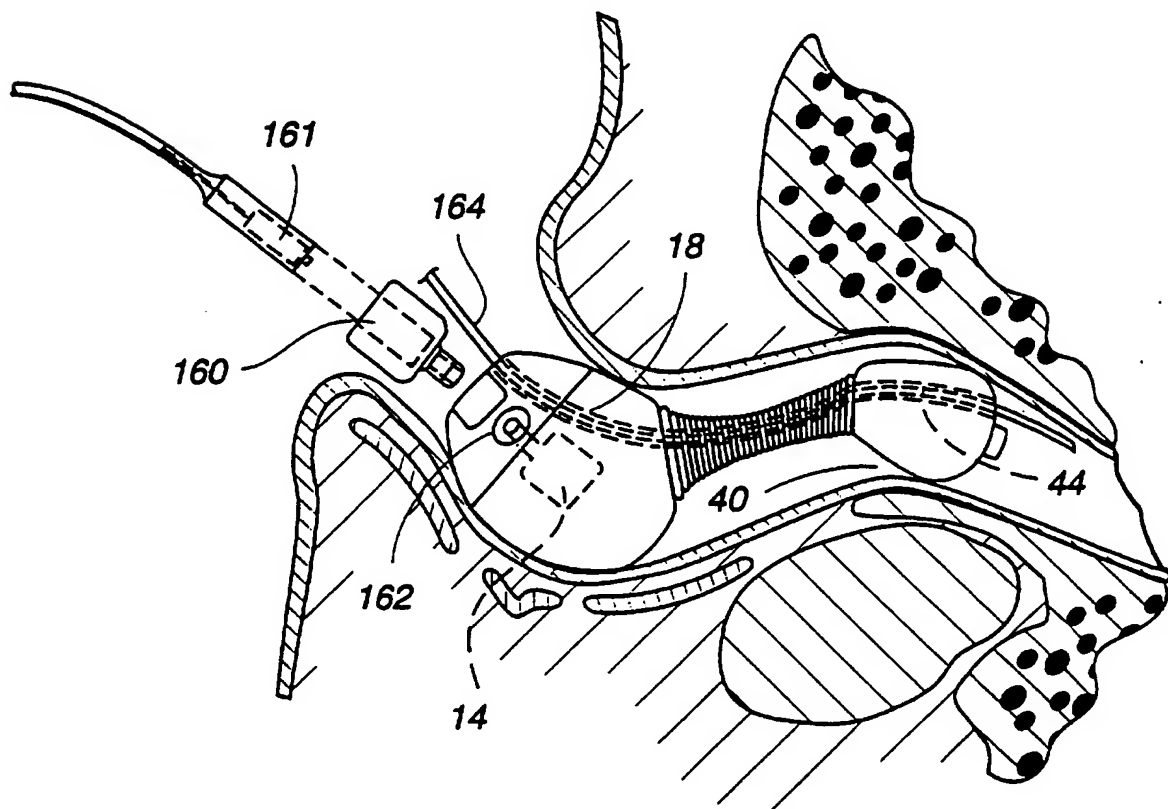
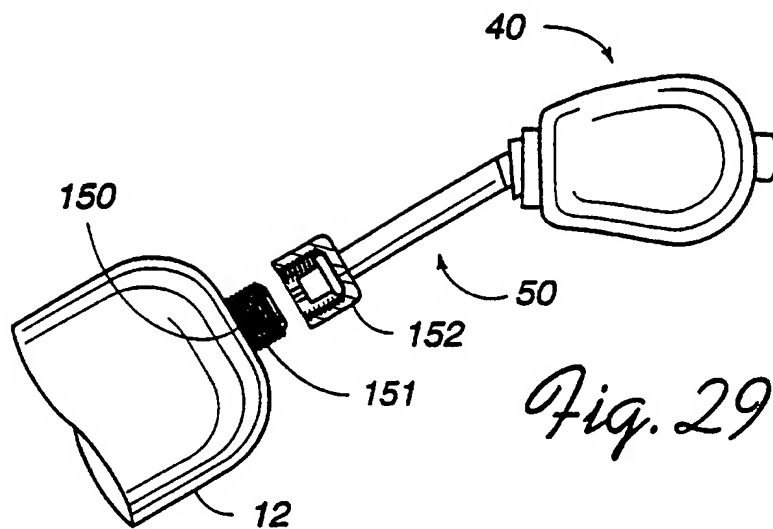


Fig. 28

13/14



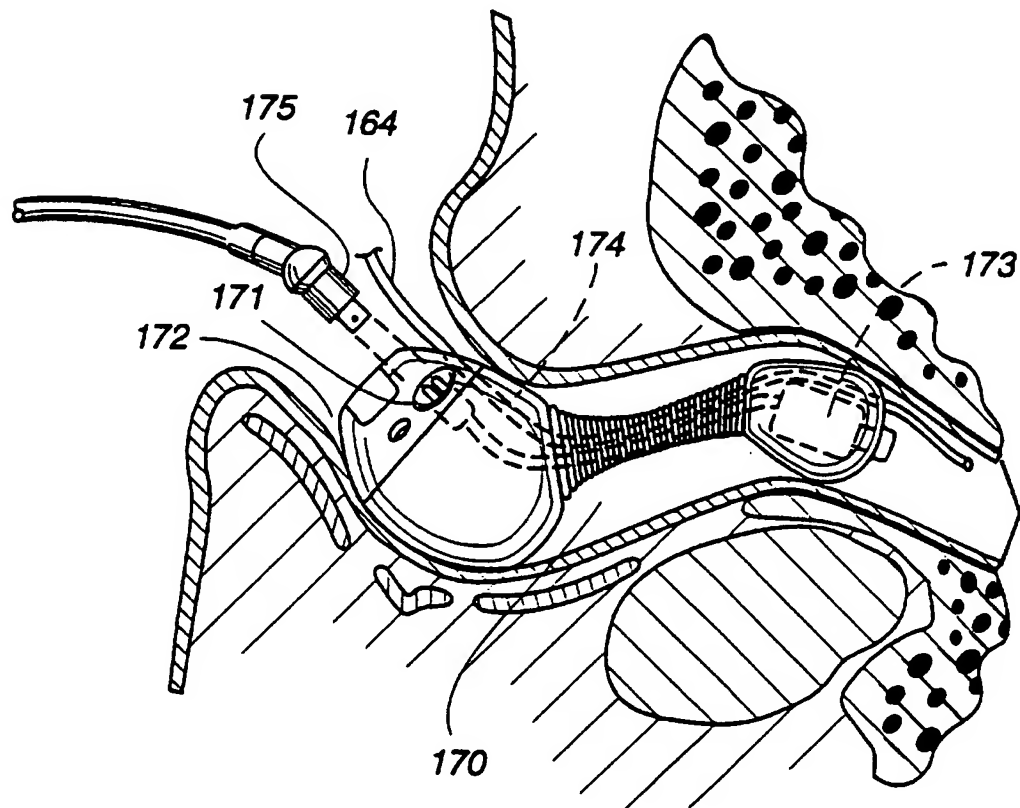


Fig. 31

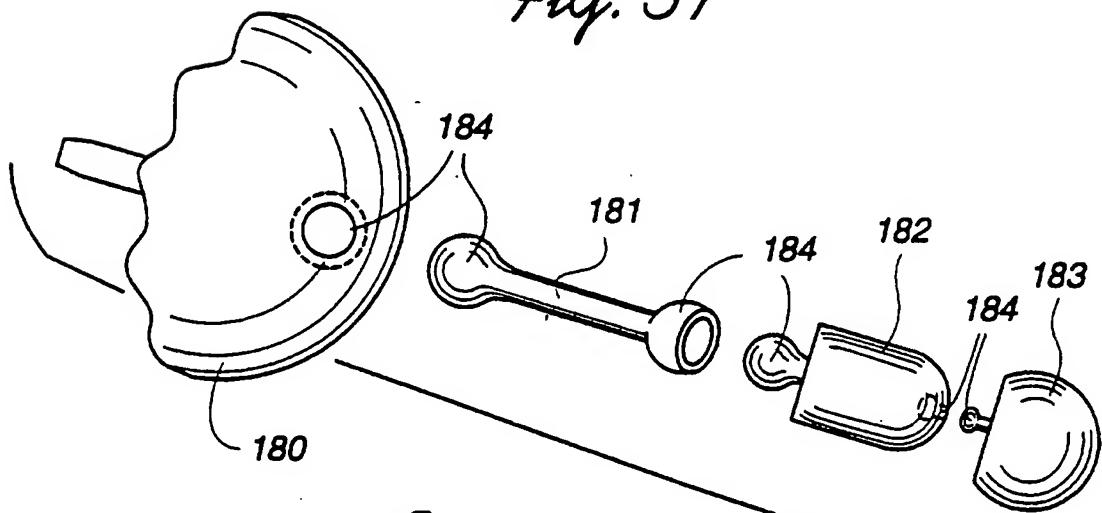


Fig. 32

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US95/17113

A. CLASSIFICATION OF SUBJECT MATTER

IPC(6) :H04R 25/00

US CL :381/68.6

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 381/68.6, 68, 68.3, 69, 69.2; 181/130, 135

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US, A, 4,937,876 (BIERMANS) 26 JUNE 1990, SEE FIGS. 1-2,	1-38
Y	GB, A, 2,203,379 (PAINTER ET AL) 19 OCTOBER 1988, SEE FIGS. 1-4 AND PAGE 3 LINE 31 - PAGE 4 LINE 11 AND PAGE 7 LINES 25-30,	1-38
Y	US, A, 5,185,802 (STANTON) 09 FEBRUARY 1993, SEE FIGS. 1,5 AND 8.	21
Y	US, A, 5,201,007 (WARD ET AL) 06 APRIL 1993, SEE FIGS. 6-7 AND COL 5 LINES 37-47 AND COL 6 LINES 50-61.	8-17, 28-31 AND 34-37

☐ Further documents are listed in the continuation of Box C.

☐ See patent family annex.

* Special categories of cited documents:	"T"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be part of particular relevance	"X"	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier document published on or after the international filing date	"Y"	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Z"	document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means		
"P" document published prior to the international filing date but later than the priority date claimed		

Date of the actual completion of the international search

17 MARCH 1996

Date of mailing of the international search report

02 APR 1996

Name and mailing address of the ISA/US
Commissioner of Patents and Trademarks
Box PCT
Washington, D.C. 20231

Facsimile No. (703) 305-3230

Authorized officer

VIVIAN CHANG

Telephone No. (703) 308-6739